

ULTRA INSTRUCTION GUIDE

Milliken™

MILLIKEN HEALTHCARE PRODUCTS, LLC




Remove

ULTRA or ULTRA Silver dressing from package. If required, dressing can be cut to size.




Apply

ULTRA with printed side of dressing away from the wound.

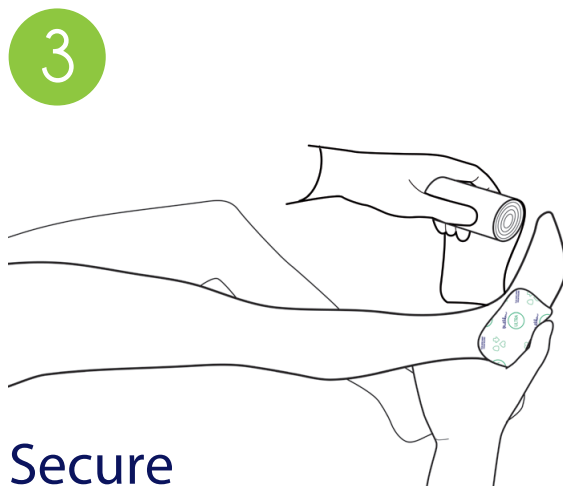

Secure

ULTRA using standard methods.

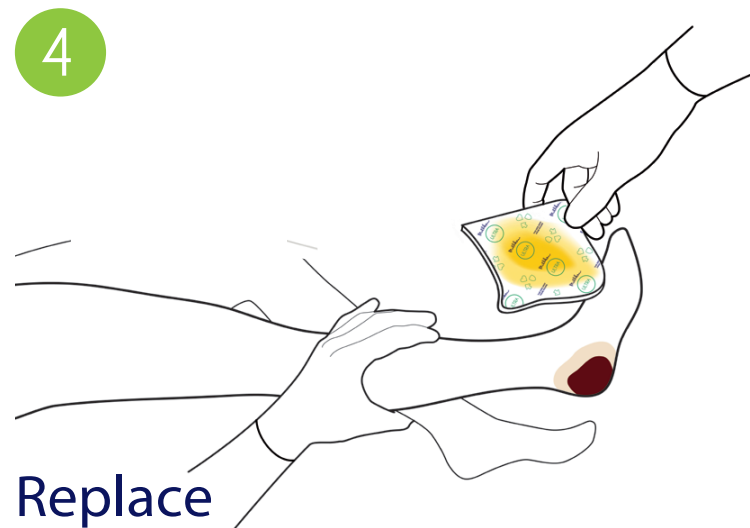

Replace

ULTRA per doctor's orders. Gently lift dressings from the wound. If needed, moisten with sterile saline or water to ease removal.